

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
29 July 2004 (29.07.2004)

PCT

(10) International Publication Number
WO 2004/062707 A1

(51) International Patent Classification⁷: **A61L 31/02,**
31/18

(21) International Application Number:
PCT/US2003/041462

(22) International Filing Date:
30 December 2003 (30.12.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
10/338,223 8 January 2003 (08.01.2003) US

(71) Applicant: **SCIMED LIFE SYSTEMS, INC.** [US/US];
One SciMed Place, Maple Grove, MN 55311-1566 (US).

(72) Inventor: **CRAIG, Charles, Horace;** 9354 Harritt Road,
Lakeside, CA 92040 (US).

(74) Agent: **GAGEL, John, J.;** Fish & Richardson P.C., 225
Franklin Street, Boston, MA 02110-2804 (US).

(81) Designated States (*national*): AE, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CR, CU, CZ, DE, DK, DM, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, UZ, VN, YU, ZA, ZW.


(84) Designated States (*regional*): ARIPO patent (BW, GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

- with international search report
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: **MEDICAL DEVICES**

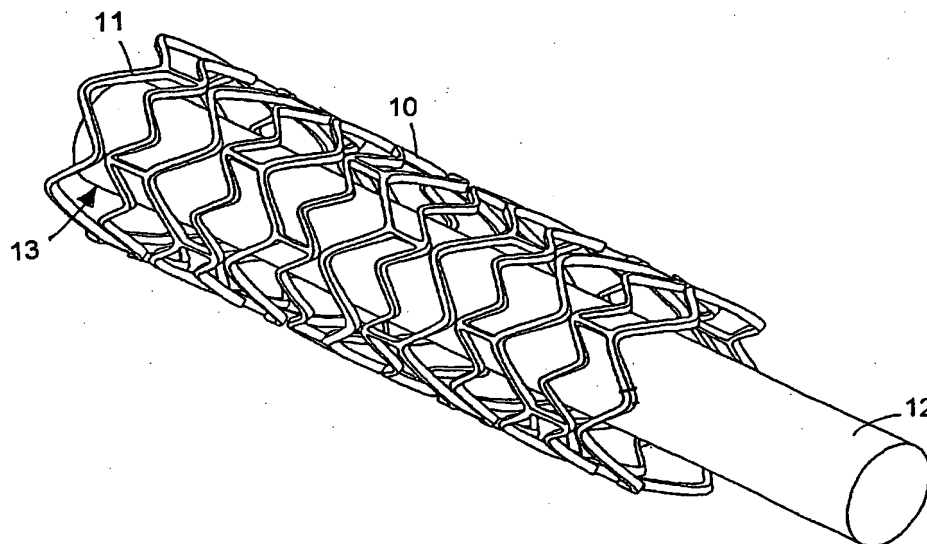

(57) Abstract: Alloy compositions suitable for fabricating medical devices, such as stents, are disclosed. In certain embodiments, the compositions have small amounts of nickel, e.g., the compositions can be substantially free of nickel.

WO 2004/062707 A1

MEDICAL DEVICES**TECHNICAL FIELD**

[0001] The invention relates to medical devices, such as, for example, stents and stent-grafts.

BACKGROUND

[0002] The body includes various passageways such as arteries, other blood vessels, and other body lumens. These passageways sometimes become occluded or weakened. For example, the passageways can be occluded by a tumor, restricted by plaque, or weakened by an aneurysm. When this occurs, the passageway can be reopened or reinforced, or even replaced, with a medical endoprosthesis. An endoprosthesis is typically a tubular member that is placed in a lumen in the body. Examples of endoprosthesis include stents and covered stents, sometimes called "stent-grafts".

[0003] Endoprostheses can be delivered inside the body by a catheter that supports the endoprosthesis in a compacted or reduced-size form as the endoprosthesis is transported to a desired site. Upon reaching the site, the endoprosthesis is expanded, for example, so that it can contact the walls of the lumen.

[0004] The expansion mechanism may include forcing the endoprosthesis to expand radially. For example, the expansion mechanism can include the catheter carrying a balloon, which carries a balloon expandable endoprosthesis. The balloon can be inflated to deform and to fix the expanded endoprosthesis at a predetermined position in contact with the lumen wall. The balloon can then be deflated, and the catheter withdrawn.

[0005] In another technique, a self-expandable endoprosthesis is formed of an elastic material that can be reversibly compacted and expanded, e.g., elastically or through a material phase transition. During introduction into the body, the endoprosthesis is restrained in a compacted condition on a catheter. Upon reaching the desired implantation site, the restraint is removed, for example, by retracting a restraining device such as an outer sheath, enabling the endoprosthesis to self-expand by its own internal elastic restoring force.

[0006] To support a passageway open, endoprostheses are made of materials, such as low-carbon, austenitic stainless steel or Nitinol (a nickel-titanium alloy), having appropriate mechanical properties, such as tensile strength and yield strength. An example of a suitable

stainless steel is UNS S31673, which is similar to AISI 316L but having a higher chromium and nickel content range. UNS S 31673 has a general composition shown in Table 1:

Table 1: Composition of UNS S31673

Element	Weight Percent
Carbon	0.030 maximum
Manganese	2.00 maximum
Phosphorus	0.025 maximum
Sulfur	0.010 maximum
Silicon	0.75 maximum
Chromium	17.00 to 19.00
Nickel	13.00 to 15.00
Molybdenum	2.25 to 3.00
Nitrogen	0.10 maximum
Copper	0.50 maximum
Iron	Balance

where the chemical composition is maintained such that $\% \text{Cr} + (3.3)(\% \text{Mo}) \geq 26.0$.

Materials such as UNS S31673, however, can be relatively radiolucent. That is, the materials may not be easily visible under X-ray fluoroscopy, a technique used to locate and to monitor the endoprostheses during and after delivery. To enhance their visibility (e.g., by increasing their radiopacity), the endoprostheses can include a relatively radiopaque material, such as gold or platinum.

SUMMARY

[0007] The invention relates to medical devices, such as, for example, stents and stent-grafts. In one aspect, the invention features a medical device including an austenitic and non-magnetic stainless steel alloy that includes a small quantity amount of nickel. For example, in some embodiments, the alloy is substantially free of nickel, which, as used herein, means that the alloy has less than about one weight percent of nickel. Nickel can cause an adverse (e.g., allergic and/or cytotoxic) effect in some subjects. At the same time, the alloy can provide the medical device with good radiopacity, tensile strength, yield strength, elongation,

and/or resistance to corrosion. In some cases, the alloy has a radiopacity, physical properties, and mechanical properties comparable or better than those of UNS S31673.

[0008] In another aspect, the invention features a medical device having an alloy including iron and chromium, being substantially free of nickel, and having a radiopacity greater than the radiopacity of UNS S31673.

[0009] In another aspect, the invention features a medical device having an alloy including iron, chromium, and less than five weight percent of nickel. The alloy is fully austenitic and has a radiopacity greater than the radiopacity of UNS S31673. The alloy can have less than five weight percent of nickel, e.g., less than four, three, two, or one weight percent of nickel.

[0010] Embodiments may include one or more of the following features. The alloy is fully austenitic. The alloy, after annealing, has a tensile strength greater than about 490 MPa. The alloy, after annealing, has a yield strength of greater than about 190 MPa. The device alloy has a pitting resistance equivalent greater than about 26. The alloy further includes one or more elements selected from platinum, ruthenium, palladium, iridium, rhodium, gold, and/or osmium. The alloy includes between about 0.5% and about 40% by weight of the first element. The device is in the form of a stent.

[0011] The alloy can have one or more of the following compositions. The alloy includes between about 0.01% and about 1.0 % by weight percent of nitrogen, e.g., less than about 1.0% by weight of nitrogen. The alloy includes between about 0.07% and about 55% by weight of cobalt, e.g., between about 0.07% and about 32% by weight of cobalt. The alloy includes between about 0.5% and about 20% by weight of manganese. The alloy includes between about 0.03% and about 6% by weight of copper. The alloy includes less than about 30% by weight of chromium, e.g., less than about 20% by weight of chromium. The alloy includes less than about 3% by weight of molybdenum.

[0012] In another aspect, the invention features a medical device having an alloy including iron, less than about 30% by weight of chromium, less than about 3% by weight of molybdenum, less than about 55% by weight of cobalt, less than about 20% by weight of manganese, less than about 6% by weight of copper, less than about 0.03% by weight of nickel, less than about 1.0% by weight of nitrogen, and between about 0.5% and about 40% by weight of a first element selected from platinum, ruthenium, palladium, iridium, rhodium, gold, and/or osmium, wherein the alloy is substantially austenitic.

[0013] The alloy can have one or more of the following compositions. The alloy includes between about 0.01% and 1.0% by weight of nitrogen. The alloy includes between about 0.07% and about 32% by weight of cobalt. The alloy includes between about 0.5% and about 20% by weight of manganese. The alloy includes between about 0.03% and about 6% by weight of copper.

[0014] In another aspect, the invention features a method of making a medical device. The method includes selecting an alloy including iron, chromium, and less than 5% by weight of nickel, wherein the alloy is substantially austenitic and has at least one of the following properties: a radiopacity greater than the radiopacity of UNS S31673, a tensile strength, after annealing, greater than about 490 MPa, a yield strength, after annealing, greater than about 190 MPa, or a pitting resistance equivalent greater than about 26; and incorporating the alloy in the medical device, such as a stent.

[0015] The alloy can have at least two of the properties, e.g., at least three of the properties. The alloy can be substantially free of nickel. The alloy can include between about 0.5% and about 40% by weight of a first element selected from platinum, ruthenium, palladium, iridium, rhodium, gold, or osmium.

[0016] In another aspect, the invention features a medical device including a nickel-free alloy having the same structure (e.g., face centered cubic) and comparable mechanical properties as a stainless steel, such as UNS S31673, conforming to ASTM F 138, F 139, and ISO 5832-1 Composition D. The alloy can have enhanced radiopacity.

[0017] The alloys described herein can also be used in dental prostheses, jewelry, flatware, or other items that can come into bodily contact.

[0018] In yet another aspect, the invention features the alloy compositions described herein.

[0019] Other aspects, features, and advantages of the invention will be apparent from the description of the preferred embodiments thereof and from the claims.

DESCRIPTION OF DRAWINGS

[0020] Fig. 1 is a perspective view of an embodiment of a stent.

[0021] Fig. 2A is a table showing the chemical compositions of four alloys; Fig. 2B is a table showing the Cr_{eq} , Ni_{eq} , and Cr_{eq}/Ni_{eq} ratios of the alloys of Fig. 2A; Fig. 2C is a table showing the microstructure and New PHACOMP calculations for the alloys of Fig. 2A; and

Fig. 2D is a table showing the calculated mechanical, corrosion, and radiopacity properties of the alloys of Fig. 2A.

[0022] Fig. 3A is a table showing the chemical compositions of six alloys; Fig. 3B is a table showing the Cr_{eq} , Ni_{eq} , and Cr_{eq}/Ni_{eq} ratios of the alloys of Fig. 3A; Fig. 3C is a table showing the microstructure and New PHACOMP calculations for the alloys of Fig. 3A; and Fig. 3D is a table showing the calculated mechanical, corrosion, and radiopacity properties of the alloys of Fig. 3A.

[0023] Fig. 4A is a table showing the chemical compositions of six alloys; Fig. 4B is a table showing the Cr_{eq} , Ni_{eq} , and Cr_{eq}/Ni_{eq} ratios of the alloys of Fig. 4A; Fig. 4C is a table showing the microstructure and New PHACOMP calculations for the alloys of Fig. 4A; and Fig. 4D is a table showing the calculated mechanical, corrosion, and radiopacity properties of the alloys of Fig. 4A.

DETAILED DESCRIPTION

[0024] Referring to Fig. 1, a support 12 carries a stent 10, which is the form of a tubular member including struts 11 and openings 13. Depending on the type of stent, e.g., balloon-expandable or self-expandable, support 12 can be a balloon catheter or a catheter shaft.

[0025] Stent 10 is composed of an alloy based on an iron-chromium stainless steel. As shown in Table 2, the alloy generally includes, among others, a small quantity of nickel, chromium, iron, and an element X:

Table 2: Composition of alloy of stent 10

Element	Weight Percent
Nickel	≤ 5.0
Chromium	15.00 - 20.00
Element X	0.50 - 40.00
Iron	balance (e.g., 40 - 65)

Element X can include one or more (e.g., two, three, four, five, six or more) of the following elements, in any combination: platinum, ruthenium, palladium, iridium, rhodium, gold, and

osmium. In addition, the alloy may include one or more of the following elements: carbon, nitrogen, manganese, copper, cobalt, and molybdenum.

[0026] As shown in Table 2, the alloy of stent 10 has a small quantity of nickel. In embodiments, the alloy has less than about five percent by weight of nickel. For example, the alloy can have less than or equal to 4%, 3%, 2%, or 1% by weight of nickel; and/or greater than or equal to 1%, 2%, 3%, or 4% by weight of nickel. Preferably, the alloy is substantially free of nickel, i.e., having less than or equal to 1% by weight of nickel (e.g., less than or equal to 0.05 or 0.03% by weight). It is believed that nickel can cause an allergic and/or cytotoxic effect in certain subjects. Therefore, by reducing the amount of nickel in the alloy of stent 10, the occurrence of the effect(s) can be reduced (e.g., minimized or eliminated).

[0027] Nickel can be used to promote a stable austenitic microstructure in a stainless steel alloy. It is believed that the austenite (face centered cubic) structure provides the alloy that is non-magnetic with good strength and ductility, which, for example, is beneficial to stent 10 because the stent can undergo considerable deformation during use. Thus, since the amount of nickel is relatively small, one or more other elements capable of promoting and/or stabilizing an austenitic microstructure ("austenitizing elements") can be added to provide a stable austenitic structure in the alloy of stent 10.

[0028] Austenitizing elements include, for example, carbon, nitrogen, manganese, copper, cobalt, and certain element X (e.g., Pt, Ir, Rh, Ru, Os, and Pd). Carbon is capable of promoting and stabilizing austenite, but at high concentrations, carbon can react to form carbides, such as iron carbides, chromium carbides, and/or molybdenum carbides. The alloy can include up to 0.03 weight percent of carbon, e.g., less than or equal to about 0.02 or 0.01 weight percent. The alloy can include greater than zero weight percent and less than about one weight percent of nitrogen, e.g., less than or equal to about 0.75, 0.50, or 0.25 weight percent. Manganese can compose up to about 20 weight percent of the alloy, e.g., less than or equal to about 15, 10, or 5 weight percent. In embodiments, such as when the alloy is used in balloon-expandable stents, the amounts of nitrogen and/or manganese are controlled so as to not significantly increase the strength, e.g., yield strength, which can hinder use of the stent. Copper, which can be an austenite promoter and/or stabilizer, can be included up to six weight percent, e.g., less than or equal to about five, four, three, two, or one weight

percent. Cobalt, which can be an austenite promoter and/or stabilizer can be includes up to 55 weight percent, e.g., less than or equal about 55, 50, 45, 40, 35, 32, 30, 25, 20, 15, 10 or 5 weight percent, and/or greater than or equal to about 5, 10, 15, 20, 25, 30, 32, 35, 40, 45, or 50 weight percent. In some cases, the alloy includes less than one weight percent of cobalt.

[0029] Molybdenum can be added to the alloy to enhance the resistance of the alloy to corrosion, e.g., pitting and crevice corrosion. In embodiments, the alloy includes between about 2.25 to about 3.00 weight percent of molybdenum, e.g., greater than or equal to 2.3, 2.4, 2.5, 2.6, 2.7, 2.8, or 2.9 weight percent, and/or less than or equal to 3.0, 2.9, 2.8, 2.7, 2.6, 2.5, 2.4, or 2.3 weight percent.

[0030] Chromium can also be added to the alloy to make the alloy more corrosion resistant. In embodiments, at 12 wt% or higher, chromium can form a thin oxide layer on the surface of a steel that enhances the resistance of the steel to corrosive attack. The degree of corrosion resistance is a function of the chromium concentration and the concentrations of other elements in the steel. The alloy can include between about 5 and about 30 weight percent of chromium. The alloy can include greater than or equal to 5, 8, 11, 14, 17, 20, 25, or 30 weight percent, and/or less than or equal to 30, 25, 20, 17, 14, 11, or 8 weight percent of chromium. Increasing the concentration of chromium can improve the pitting resistance, e.g., to be equal to or better than UNS S31673. But in some cases, the higher the chromium concentration, the more austenitizing elements and/or stabilizers, such as Co, Mn, N, and/or Cu, may be required to maintain an austenitic structure.

[0031] Element X is selected from a group of elements capable of enhancing the radiopacity of the alloy. Element X can be a face-centered-cubic element. In embodiments, element X has a density equal to or greater than about 2 g/cc, e.g., equal to or greater than 9.9 g/cc. The alloy can include between about 0.5 and about 40 weight percent of element X. The alloy can include greater than or equal to about 5, 10, 15, 20, 25, 30, or 35 weight percent, and/or less than or equal to about 40, 35, 30, 25, 20, 15, 10, or 5 weight percent of element X. In some cases, such as when element X is rhodium, iridium, palladium, ruthenium, osmium, or platinum, element X can also promote and/or stabilize the austenite structure.

[0032] The alloy can include residual amounts of impurities elements. For example, the alloy may include residual amounts of phosphorus (e.g., 0.025 wt% maximum), silicon (e.g. 0.75 wt% maximum), sulfur (e.g., 0.010 wt% maximum), niobium (e.g., about 0.013 wt%),

vanadium (e.g., about 0.07 wt%), titanium (e.g., 0.002 wt%), and/or aluminum (e.g., about 0.009 wt%). Other residual elements and residual amounts are possible, which can be a function of the source of the materials.

[0033] Iron makes up the balance of the alloy of stent 10, e.g., after accounting for the other elements in the alloy described above. In certain embodiments, the alloy includes between about 40 and about 65 weight percent of iron.

[0034] Particular compositions of the alloy are selected to provide the alloy with one or more selected physical and mechanical properties, such as radiopacity, strength, elongation, and resistance to corrosion, suitable for intravascular use. In embodiments, the physical and mechanical properties are comparable to or better than those of other stainless steels, such as UNS S31673, used in medical devices. Without wishing to be bound by theory, it is believed that these properties can be modeled to help predict, and therefore, target, compositions can provide the selected properties. For example, a particular composition can be analyzed to determine theoretically whether it can form a selected phase, such as austenite. Similarly, the composition can be modeled to determine theoretically whether it can have suitable mechanical and physical properties for medical applications.

[0035] Microstructure: In some embodiments, the alloy has a microstructure that is predominantly (greater than 50%) austenitic, i.e., the alloy is formed predominantly of the austenite phase. For example, the alloy can be equal to or greater than 80%, 85%, 90%, or 95% austenitic. Preferably, the alloy is fully austenitic. As discussed above, it is believed that the austenite structure can provide a non-magnetic alloy with good strength and ductility, e.g., suitable for stent applications.

[0036] The microstructure of an alloy can be predicted using constitutional diagrams, such as the Schaeffler diagram and the Welding Research Council (WRC-1988) diagram. (See ASM International, ASM Speciality Handbook: Stainless Steels, Welding, pp. 340-342, Davis J.R. Library on Congress Cataloging-In-Publication Data, 1994; Siewert et al., Ferrite Number Prediction to 100FN in Stainless Steel Weld Metal, Weld. J., Vol. 67 No. 12, 1988, pp. 289s-298s; and Hull, Delta Ferrite and Martensite Formation in Stainless Steels, Welding Research Supplement, May 1973, pp. 193-203.) The Schaeffler diagram predicts the phases in the alloy, and the WRC diagram provides more detail in the range under consideration. In

particular, the phase to which the alloy solidifies can be dependent on the chromium equivalent to nickel equivalent ratio (Cr_{eq}/Ni_{eq}), in which:

$$Cr_{eq} = (\%Cr) + (\%Mo) + (1.5)(\%Si) + (0.5)(\%Nb)$$

$$Ni_{eq} = (\%Ni) + (30)(\%C) + (0.5)(\%Mn)$$

For a Cr_{eq}/Ni_{eq} ratio approximately 1.48 or less, the composition can solidify as austenite; for a Cr_{eq}/Ni_{eq} ratio approximately between 1.48 and 1.95, the composition can solidify as a duplex structure of austenite and ferrite; and for a Cr_{eq}/Ni_{eq} ratio approximately 1.95 or greater, the composition can solidify as ferrite. In embodiments, it is desirable for the composition to solidify in the austenite (A) phase or the austenite-ferrite (AF) phase, which is mostly austenite. In the ferrite (F) phase or ferrite-austenite (FA) phase (which is mostly ferrite), the solubility of nitrogen (which can increase austenite formation and stability) can decrease as the composition solidifies, resulting in increased porosity.

[0037] Austenite stability at ambient temperature can also reduce the occurrence of martensite formation in the alloy during cold forming operations. Uncontrolled transformation of austenite to martensite can make the alloy magnetic, can lead to dimensional instability, and can be the dominant cause of work hardening, e.g., reduced ductility. The martensite deformation temperature, M_d , can be the temperature at which 50% of martensite is formed by 30% deformation. M_d can be calculated as follows:

$$M_d (^\circ C) = 13 - 462(C + N) - 9.2Si - 8.1Mn - 13.7Cr - 9.5Ni - 18.5Mo - 18.5Cu \\ - 10(Ru + Rh + Pd + Ir + Pt + Au)$$

For more information, see Angel T., Formation of Martensite in Austenitic Stainless Steels: Effects of Deformation, Temperature, and Composition, Journal of the Iron and Steel Institute, May 1954, pp. 165-174. In embodiments, the austenite phase in the alloy is stable at high and low temperatures, and the formation of the intermetallic phases at grain boundaries is reduced (e.g. minimized). In certain embodiments, M_d is well below zero degrees Celsius.

[0038] TCP Phases and Nitrogen Concentration: In embodiments, the alloy includes reduced (e.g., minimal or no) amounts of brittle topologically close packed (TCP) phases. A phase computational methodology, called "New PHACOMP" (Morinaga et al., Solid Solubilities in Transition-Metal-Base FCC Alloys, Philosophical Magazine A, 1985, Vol. 51, No. 2, pp.

223-246), can be used to help predict the tendency of austenite to precipitate TCP phases, e.g., sigma (σ) phases in nickel-based alloys, and cobalt and iron based superalloys.

[0039] In New PHACOMP, the d orbital energy level (Md) of an element is used to calculate the average Md (Md^{ave}) for the composition using the formula:

$$Md^{ave} (eV) = \sum X_i (Md)_i$$

where X_i is the atomic fraction of element i in the composition, and $(Md)_i$ is the Md of element i . The summation is taken over all the elements of the alloy.

[0040] It is believed that when Md^{ave} becomes larger than a critical value (Md^{crit}), phase instability can occur and a second phase, i.e., a TCP phase, is formed in the austenite matrix. Md^{crit} is a function of the second phase. Here, for compositions containing $\leq 0.06\%$ nitrogen:

$$Md^{crit} (eV) = 0.834 + (6.25 \times 10^{-5})T$$

where T is the temperature in Kelvin. For compositions containing $> 0.06\%$ nitrogen:

$$Md^{crit} (eV) = 0.834 + (6.25 \times 10^{-5})T + 0.02N_{max}$$

More information can be found in Uggowitzer et al., High Nitrogen Austenitic Stainless Steels – Properties and New Developments, Innovation Stainless Steel, Florence, Italy, 11-14 October 1993.

[0041] In embodiments, the alloy has an Md^{ave} value equal to or greater than Md^{crit} , e.g., greater than by 0.002 eV.

[0042] In addition, New PHACOMP can be used to predict precipitation of chromium nitride in relatively high-nitrogen stainless steels (e.g., as described in Uggowitzer et al.). As discussed above, nitrogen can be added to austenitic steels to stabilize austenite, e.g., by reducing the occurrence of ferrite formation at high temperatures and martensitic transformation at low temperatures. In certain cases, when the nitrogen content exceeds its solubility limit in austenite, chromium nitride (e.g., Cr_2N) can precipitate and deplete the matrix of chromium, thereby reducing passivity.

[0043] The Md^{ave} value (above) can be used to calculate this solubility limit. The solubility of nitrogen in the austenite phase can vary, e.g., as a function of the composition. In embodiments, the estimated solubility limit at annealing temperatures (e.g., about 1050 °C) is

similar to that obtained after quenching. A formula to predict the maximum amount of nitrogen that can dissolve in austenite before chromium nitride precipitates, $N_{\max}(\%)$, is:

$$N_{\max}(\%) = 0.003 \exp \{41660[(M_d^{\text{ave}} - 0.75)/(2765 - T)]\}$$

where T is the temperature in Kelvin. More information can be found at Uggowitzer et al. In certain embodiments, the alloy has a nitrogen concentration equal to or less than $N_{\max}(\%)$ to reduce the occurrence of chromium nitride precipitation.

[0044] **Radiopacity:** The alloy is preferably radiopaque. The radiopacity of the alloy can be enhanced by including one or more element X (e.g., Pt, Ir, Os, Re, Rh, Pd, Ru, and Au). Element(s) X that are good austenite formers can also reduce the amount of other austenite forming or stabilizing elements (see above).

The effect of an element on the radiopacity of an alloy is dependent on the relative proportion of the element, and the mass attenuation coefficient of the element. The mass attenuation coefficient (μ/ρ) for each element at various energy levels can be obtained from <http://physics.nist.gov/>. (See, e.g., Hubbell, J. H. and Seltzer, S. M. (1997). *Tables of X-Ray Mass Attenuation Coefficients and Mass Energy-Absorption Coefficients* (version 1.03), available at <http://physics.nist.gov/xaamdi> [2002, November 5]. National Institute of Standards and Technology, Gaithersburg, MD, which was originally published as NISTIR 5632, National Institute of Standards and Technology, Gaithersburg, MD (1995). See, also, NISTIR 5632, *Tables of X-Ray Mass Attenuation Coefficients and Mass Energy-Absorption Coefficients 1 keV to 20 MeV for Elements Z = 1 to 92 and 48 Additional Substances of Dosimetric Interest*, Published date: May 1995.)

[0045] The linear attenuation coefficient of an element, at a certain energy level, can be derived by multiplying its mass attenuation coefficient by its density. The average mass attenuation coefficient $(\mu/\rho)_{\text{ave}}$ of an alloy can be obtained by multiplying the elemental mass attenuation coefficient (μ/ρ) by the weight fraction of each element in the alloy, and summing the contribution of each element:

$$\left(\frac{\mu}{\rho}\right)_{\text{ave}} = \sum_{i=1}^n (wt\%)_i \cdot \left(\frac{\mu}{\rho}\right)_i$$

[0046] The average density for the alloy can be calculated as:

$$\frac{1}{\rho} = \sum_i \left(\frac{c_i}{\rho_i} \right)$$

where c_i is the mass percent of element i , and ρ_i is the density of pure element i .

The average linear attenuation coefficient $(\mu)_{ave}$ for the alloy can then be obtained by multiplying the average mass attenuation coefficient by the average density. The radiopacity at a certain energy level can be derived as:

$$Radiopacity = e^{\mu_{ave} x}$$

where μ_{ave} is the average linear attenuation coefficient, and x is the thickness of the alloy. Methods of calculating the radiopacity of an alloy at a certain energy level are also described in Craig et al., Development of a Platinum-Enhanced Radiopaque Stainless Steel (PERSS®), Stainless Steel for Medical and Surgical Applications, ASTM STP 1438, G.L. Winters and M.J. Nutts, Eds., ASTM International, Pittsburgh, PA, 2002.

[0047] The radiopacity of the alloy is dependent on the incident energy and the thickness of the alloy. In embodiments, for an alloy sample, 0.005" (0.127 mm) thick, at an incident energy level of 40 keV, the alloy of stent 10 has a radiopacity of equal to or greater than about 1.539. At an incident energy level of 60 keV, the alloy of stent 10 can have a radiopacity of equal to or greater than about 1.156. At an incident energy level of 80 keV, the alloy of stent 10 can have a radiopacity of equal to or greater than about 1.118. At an incident energy level of 100 keV, the alloy of stent 10 can have a radiopacity of equal to or greater than about 1.069

[0048] For purposes of comparison, a stainless steel, such as UNS S31673 (0.005" thick"), has a radiopacity of 1.475 at 40 keV, 1.138 at 60 keV, 1.066 at 80 keV, and 1.040 at 100 keV. These values are median values and can vary, depending on the particular composition.

[0049] In some embodiments, the alloy has a radiopacity greater than or equal to about 105%, 110%, 115%, 120%, or 125% of the radiopacity of UNS S31673 at 80 keV for a thickness of 0.005 inch; and/or less than or equal to about 130%, 125%, 120%, 115%, 110%, or 105% of the radiopacity of UNS S31673 at 80 keV for a thickness of 0.005 inch.

[0050] Mechanical Properties: The mechanical properties of an alloy can be estimated as follows.

$$\begin{aligned} \text{Tensile strength (MPa)} = & 470 + 600(N+0.02) + 14\text{Mo} + 1.5\delta + 8d^{-0.5} + 20\text{Ru} + 7\text{Rh} \\ & + 9\text{Pt} + 7\text{Ir} + 12\text{Pd} + 5\text{Au} \end{aligned}$$

$$\begin{aligned} \text{Yield strength (MPa)} = & 120 + 210(N+0.02) - 0.5 + 2\text{Cr} + 2\text{Mn} + 14\text{Mo} + 10\text{Cu} + \delta(6.15 - \\ & 0.054\delta) + (7 + 35(N+0.02))d^{-0.5} \end{aligned}$$

where d is the grain size (in mm), and δ is the delta ferrite content (in volume percent). In embodiments, d can be set at 0.04 mm and δ can be set at zero percent. For more information, see Nordberg, Mechanical Properties of Austenitic and Duplex Stainless Steels, Innovation Stainless Steel, Florence, Italy, 11-14 October 1993, Vol. 2, pp. 2.217-2.229; and Uggowitzer et al., Strengthening of Austenitic Stainless Steels by Nitrogen, HNS – 88.

[0051] In some embodiments, the alloy (after annealing) has a tensile strength of equal to or greater than 490 MPa, e.g., greater than about 500, 600, 700, or 800 MPa. Alternatively or in addition, the alloy (after annealing) can have a yield strength of equal to or greater/less than 190 MPa, e.g., greater than about 200, 300, or 400 MPa. Alternatively or in addition, the alloy (after annealing) can have an elongation equal to or greater than about 40%.

[0052] Corrosion Resistance: The corrosion resistance properties can also be estimated. In embodiments, a pitting resistance equivalent (PRE) of an alloy is greater than or equal to 26 (e.g., for ASTM F 138 and 139, and ISO5832-1). The pitting resistance equivalent can be predicted by using the formula:

$$\text{PRE} = \text{Cr} + 3.3\text{Mo} + 16\text{N}$$

which accounts for the effect of nitrogen, which can have a beneficial effect on pitting resistance. More information can be found in Gunn, Duplex Stainless Steels, Woodhead Publishing Limited, England, 1997, pp. 84.

[0053] In embodiments, the alloy has a pitting resistance equivalent equal to or greater than about 26.

[0054] By using the models and methodologies described above, different compositions of alloys can be studied to determine whether a composition can provide one or more selected properties. For example, the models and methodologies can be entered into a software program. A user can input a selected composition, and the program can output the predicted

properties of the composition, e.g., in tabular or graphical form. The user can select those compositions having predetermined, predicted properties. The selected composition can have one or more (e.g., two, three, four, five, or more) of the properties described above, in any combination.

[0055] The following examples are illustrative and not intended to be limiting.

[0056] Examples

[0057] Figs. 2A-2D, 3A-3D, and 4A-D show seventeen alloy compositions (Alloys A-Q) and their physical, microstructural, and mechanical properties, predicted using the models and methodologies described above.

[0058] All of the compositions have Cr_{eq}/Ni_{eq} ratios of 1.48 or less, which indicate that the compositions can solidify to a phase containing an austenite phase. All of the compositions also have low martensite deformation temperatures, M_d , e.g., less than zero degrees Celsius.

[0059] New PHACOMP analyses indicate all of the alloys, except Alloys I and K-O should not precipitate sigma phases (TCP phases) because Md^{ave} is less than Md^{crit} . Alloys L and M are predicted to precipitate sigma phases. For Alloys I, K, N, and O, the tendency of the alloy to precipitate TCP phases is borderline because the difference between Md^{ave} and Md^{crit} is less than 0.002. New PHACOMP analyses also indicate no precipitation of chromium nitride in the alloys because the nitrogen concentrations are less than the maximum amounts of nitrogen solubility, N_{max} .

[0060] The predicted mechanical, corrosion, and radiopacity properties are shown in Figs. 2D, 3D, and 4D.

[0061] Selected alloy compositions were manufactured using high-purity raw materials. The materials were melted in a button arc furnace in a water-cooled copper hearth under an argon atmosphere of approximately 0.3 of an atmospheric pressure. The materials were homogenized by melting three times, with turning between each melt. The alloys were then annealed in a vacuum furnace, at between 1050 °C and 1150 °C for about two hours.

[0062] Stent 10 can be formed by folding and welding a sheet or a foil of the alloy to provide a tube, e.g., using inert gas or electron beam methods, with appropriate protection against oxidation. The tube can then be drawn or extruded to the desired diameter, or used to fabricate a stent directly. Alternatively, a thin-walled tube of the alloy can be used. Portions

of the tube can be removed to provide the strut 11/opening 13 arrangement. The portions can be removed by laser cutting, as described, for example, in U.S. Pat. 5,780,807. Alternatively, the portions can be removed by electrochemical machining, electrical discharge machining, abrasive cutting/grinding methods, or photoetching. Stent 10 can then be finished by electropolishing to a smooth finish, by conventional methods. Stent 10 also can be annealed. In other embodiments, stent 10 is made from a flat pattern that is then formed into a tubular shape by rolling the pattern to bring opposing edges together. The edges can then be joined, e.g., by welding.

[0063] In general, stent 10 can be of any desired shape and size (e.g., coronary stents, aortic stents, peripheral stents, gastrointestinal stents, urology stents, and neurology stents). Depending on the application, stent 10 can have a diameter of between, for example, 1 mm to 46 mm. In certain embodiments, a coronary stent can have an expanded diameter of from about 2 mm to about 6 mm. In some embodiments, a peripheral stent can have an expanded diameter of from about 5 mm to about 24 mm. In certain embodiments, a gastrointestinal and/or urology stent can have an expanded diameter of from about 6 mm to about 30 mm. In some embodiments, a neurology stent can have an expanded diameter of from about 1 mm to about 12 mm. An abdominal aortic aneurysm (AAA) stent and a thoracic aortic aneurysm (TAA) stent can have a diameter from about 20 mm to about 46 mm. Stent 10 can be balloon-expandable, self-expandable, or a combination of both (e.g., as described in U.S. Patent No. 5,366,504).

[0064] Stent 10 can be used, e.g., delivered and expanded, according to conventional methods. Suitable catheter systems are described in, for example, Wang U.S. 5,195,969, and Hamlin U.S. 5,270,086. Suitable stents and stent delivery are also exemplified by the NIR on Ranger® system, available from Boston Scientific Scimed, Maple Grove, MN.

[0065] Other Embodiments

[0066] In other embodiments, stent 10 can include and/or be attached to a biocompatible, non-porous or semi-porous polymer matrix made of polytetrafluoroethylene (PTFE), expanded PTFE, polyethylene, urethane, or polypropylene. Stent 10 can include a releasable therapeutic agent or a pharmaceutically active compound, such as described in U.S. Patent No. 5,674,242, commonly-assigned U.S.S.N. 09/895,415, filed July 2, 2001, and U.S.S.N.

10/112,391, filed March 28, 2002. The therapeutic agents or pharmaceutically active compounds can include, for example, anti-thrombogenic agents, antioxidants, anti-inflammatory agents, anesthetic agents, anti-coagulants, and antibiotics.

[0067] The alloy described above can also be used in other medical devices, e.g., endoprotheses. For example, the alloy can be used in filters such as removable thrombus filters described in Kim et al., U.S. Pat. 6,146,404; in intravascular filters such as those described in Daniel et al., U.S. Pat. 6,171,327; and vena cava filters such as those described in Soon et al., U.S. Pat. 6,342,062.

[0068] The alloy can also be used in guidewires such as a Meier Steerable Guide Wire (for AAA stent procedure) and an ASAP Automated Biopsy System described in U.S. Pat. 4,958,625, 5,368,045, and 5,090,419.

[0069] All publications, references, websites, applications, and patents referred to herein are incorporated by reference in their entirety.

[0070] Other embodiments are within the claims.

What is Claimed Is:

1. A medical device, comprising:
an alloy comprising iron and chromium, the alloy being substantially free of nickel and having a radiopacity greater than the radiopacity of UNS S31673.
2. The device of claim 1, wherein the alloy is fully austenitic.
3. The device of claim 1, wherein the radiopacity is greater than about 105% of the radiopacity of UNS S31673 at 80 keV for a thickness of 0.005 inch.
4. The device of claim 1, wherein the radiopacity is greater than about 110% of the radiopacity of UNS S31673 at 80 keV for a thickness of 0.005 inch.
5. The device of claim 1, wherein the radiopacity is greater than about 115% of the radiopacity of UNS S31673 at 80 keV for a thickness of 0.005 inch.
6. The device of claim 1, wherein the radiopacity is greater than about 120% of the radiopacity of UNS S31673 at 80 keV for a thickness of 0.005 inch.
7. The device of claim 1, wherein the radiopacity is greater than about 125% of the radiopacity of UNS S31673 at 80 keV for a thickness of 0.005 inch.
8. The device of claim 1, wherein the alloy, after annealing, has a tensile strength greater than about 490 MPa.
9. The device of claim 1, wherein the alloy, after annealing, has a yield strength of greater than about 190 MPa.
10. The device of claim 1, wherein the alloy has a pitting resistance equivalent greater than about 26.

11. The device of claim 1, wherein the alloy further comprises a first element selected from a group consisting of platinum, ruthenium, palladium, iridium, rhodium, gold, and osmium.

12. The device of claim 11, wherein the alloy comprises a plurality of first elements.

13. The device of claim 11, wherein the alloy comprises between about 0.5% and about 40% by weight of the first element.

14. The device of claim 1, in the form of a stent.

15. A medical device, comprising:
an alloy comprising iron, chromium, and less than five weight percent of nickel, the alloy being fully austenitic and having a radiopacity greater than the radiopacity of UNS S31673.

16. The device of claim 15, wherein the alloy comprises less than about three weight percent of nickel.

17. The device of claim 15, wherein the alloy comprises less than about one weight percent of nickel.

18. The device of claim 15, wherein the radiopacity is greater than about 105% of the radiopacity of UNS S31673 at 80 keV for a thickness of 0.005 inch.

19. The device of claim 15, wherein the radiopacity is greater than about 110% of the radiopacity of UNS S31673 at 80 keV for a thickness of 0.005 inch.

20. The device of claim 15, wherein the radiopacity is greater than about 115% of the radiopacity of UNS S31673 at 80 keV for a thickness of 0.005 inch.

21. The device of claim 15, wherein the radiopacity is greater than about 120% of the radiopacity of UNS S31673 at 80 keV for a thickness of 0.005 inch.

22. The device of claim 15, wherein the radiopacity is greater than about 125% of the radiopacity of UNS S31673 at 80 keV for a thickness of 0.005 inch.

23. The device of claim 15, wherein the alloy further comprises between about 0.01% and about 1.0 % by weight percent of nitrogen.

24. The device of claim 15, wherein the alloy further comprises between about 0.07% and about 55% by weight of cobalt.

25. The device of claim 15, wherein the alloy further comprises between about 0.07% and about 32% by weight of cobalt.

26. The device of claim 15, wherein the alloy further comprises between about 0.5% and about 20% by weight of manganese.

27. The device of claim 15, wherein the alloy further comprises between about 0.03% and about 6% by weight of copper.

28. The device of claim 15, wherein the alloy further comprises a first element selected from a group consisting of platinum, ruthenium, palladium, iridium, rhodium, gold, and osmium.

29. The device of claim 28, wherein the alloy comprises a plurality of first elements.

30. The device of claim 28, wherein the alloy comprises between about 0.5% and about 40% by weight of the first element.
31. The device of claim 15, wherein the alloy, after annealing, has a tensile strength greater than about 490 MPa.
32. The device of claim 15, wherein the alloy, after annealing, has a yield strength of greater than about 190 MPa.
33. The device of claim 15, wherein the alloy has a pitting resistance equivalent greater than about 26.
34. The device of claim 15, wherein the alloy comprises less than about 30% by weight of chromium.
35. The device of claim 15, wherein the alloy comprises less than about 20% by weight of chromium.
36. The device of claim 15, wherein the alloy further comprises less than about 3% by weight of molybdenum.
37. The device of claim 15, wherein the alloy further comprises less than about 1.0% by weight of nitrogen.
38. The device of claim 15, in the form of a stent.
39. A medical device, comprising:
an alloy comprising
iron,
less than about 30% by weight of chromium,
less than about 3% by weight of molybdenum,

less than about 55% by weight of cobalt,
less than about 20% by weight of manganese,
less than about 6% by weight of copper,
less than about 0.03% by weight of nickel,
less than about 1.0% by weight of nitrogen, and
between about 0.5% and about 40% by weight of a first element selected
from a group consisting of platinum, ruthenium, palladium, iridium, rhodium, gold, and
osmium,
the alloy being substantially austenitic.

40. The device of claim 39, in the form of a stent.
41. The device of claim 39, comprising a plurality of first elements.
42. The device of claim 39, wherein the alloy comprises between about 0.01%
and 1.0% by weight of nitrogen.
43. The device of claim 39, wherein the alloy comprises between about 0.07%
and about 32% by weight of cobalt.
44. The device of claim 39, wherein the alloy comprises between about 0.5%
and about 20% by weight of manganese.
45. The device of claim 39, wherein the alloy comprises between about 0.03%
and about 6% by weight of copper.
46. A method of making a medical device, the method comprising:
selecting an alloy comprising iron, chromium, and less than 5% by weight
of nickel, the alloy being substantially austenitic and having at least one of the following
properties:
 - (a) a radiopacity greater than the radiopacity of UNS S31673,

(b) a tensile strength, after annealing, greater than about 490 MPa,
(c) a yield strength, after annealing, greater than about 190 MPa, or
(d) a pitting resistance equivalent greater than about 26,
incorporating the alloy in the medical device.

47. The method of claim 46, wherein the alloy has at least two of the properties.

48. The method of claim 46, wherein the alloy has at least three of the properties.

49. The method of claim 46, wherein the alloy is substantially free of nickel.

50. The method of claim 46, wherein the alloy comprises between about 0.5% and about 40% by weight of a first element selected from a group consisting of platinum, ruthenium, palladium, iridium, rhodium, gold, and osmium.

51. The method of claim 46, wherein the device is a stent.

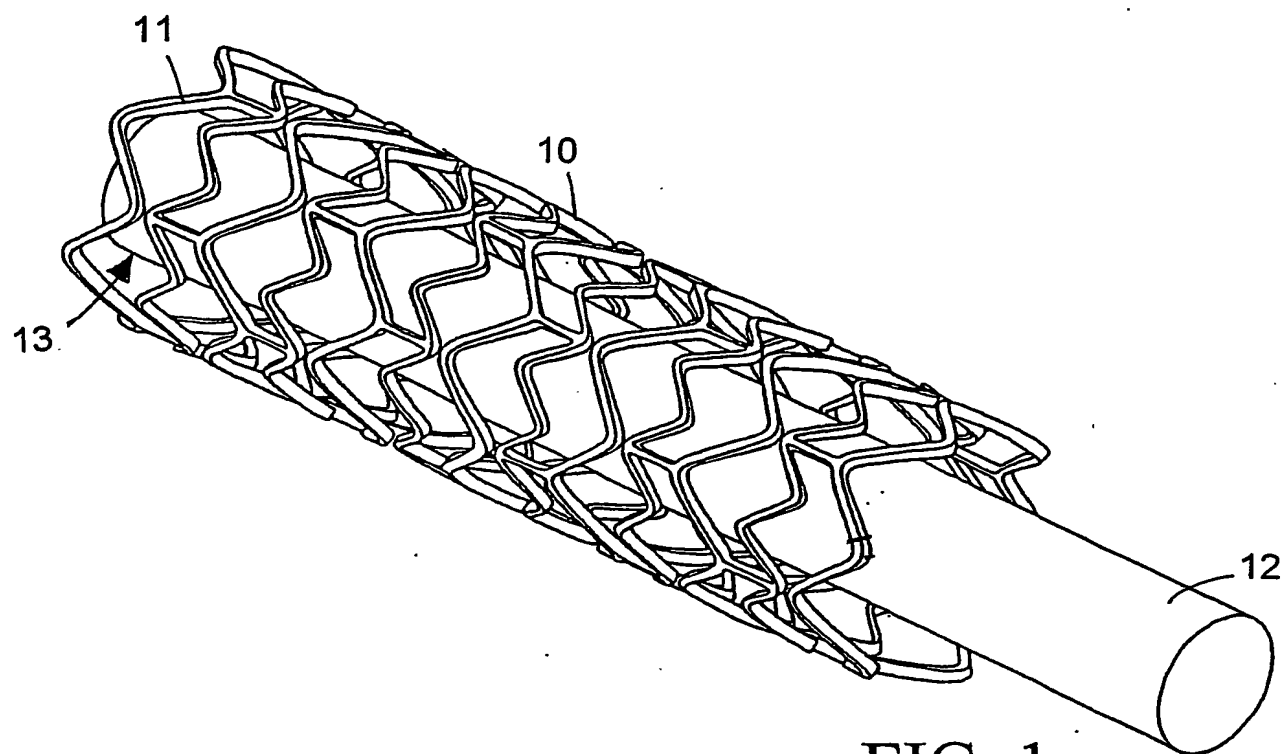


FIG. 1

Alloy	Elemental Composition (wt. %)											
	Ni	Cr	Mn	C	Mo	Si	N	Co	Pt	Ru	Pd	Ir
Alloy A	0	16	8	0.03	2.3	0.2	0.16	0.07	6	1.5	0	0
Alloy B	0	16	8	0.03	2.3	0.2	0.16	0.07	6	0	1	0
Alloy C	0	16	8	0.03	2.3	0.2	0.16	0.07	0	1.5	0	6
Alloy D	0	16	8	0.03	2.3	0.2	0.16	0.07	0	0	1.5	6

FIG. 2A

Alloy	Cr Equivalent	Ni Equivalent	Cr _{eq} /Ni _{eq}
Alloy A	19.0	13.8	1.38
Alloy B	19.0	13.6	1.40
Alloy C	19.0	13.5	1.41
Alloy D	19.0	13.4	1.41

FIG. 2B

Alloy	As Cast Microstructure			New PHACOMP Analysis (Annealing Temp = 1050°C)				
	% δ (DeLong)	Mode	M _d Temp (°C)	Cr ₂ N Phase	σ Phase	Md ^{ave} (eV)	Md ^{crit} (eV)	Max N Sol. (%)
Alloy A	1	AF	-115.2	No	No	0.920	0.925 (2)	0.41
Alloy B	2	AF / FA	-110.2	No	No	0.918	0.924 (2)	0.39
Alloy C	2	AF / FA	-115.2	No	No	0.923	0.926 (2)	0.44
Alloy D	2	AF / FA	-115.2	No	No	0.921	0.925 (2)	0.42

FIG. 2C

Alloy	Mechanical (Annealed - 1050°C)		Corrosion PRE	Radiopacity Change from 316LS (Thickness = 0.005")			
	Yield Strength (MPa)	UTS (MPa)		40 keV (%)	60 keV (%)	80 keV (%)	100 keV (%)
Alloy A	376	734	26.2	+6.4	+2.2	+5.3	+3.0
Alloy B	376	716	26.2	+5.9	+2.1	+5.2	+2.9
Alloy C	376	722	26.2	+6.1	+2.1	+5.2	+2.9
Alloy D	376	710	26.2	+6.4	+2.2	+5.2	+2.9

FIG. 2D

Alloy	Elemental Composition (wt. %)											
	Ni	Cr	Mn	C	Mo	Si	N	Co	Pt	Ru	Pd	Ir
Alloy E	0	17	8	0.03	2.6	0.2	0.22	0.07	6	0	0	0
Alloy F	0	17	8	0.03	2.6	0.2	0.22	0.07	0	0	0	6
Alloy G	0	18	1.5	0.03	2.8	0.2	0.06	24	6	0	0	0
Alloy H	0	18	1.5	0.03	2.8	0.2	0.06	24	0	0	0	6
Alloy I	0	18	1.5	0.03	2.8	0.2	0.06	17	12.5	0	0	0
Alloy J	0	17	6	0.03	2.6	0.2	0.16	0.07	12.5	0	0	0
Alloy K	0	17	6	0.03	2.6	0.2	0.16	0.07	0	0	0	12.5

FIG. 3A

Alloy	Cr Equivalent	Ni Equivalent	Cr _{eq} /Ni _{eq}
Alloy E	20.3	15.0	1.35
Alloy F	20.3	14.7	1.38
Alloy G	21.5	16.1	1.33
Alloy H	21.5	15.8	1.36
Alloy I	21.5	16.3	1.32
Alloy J	20.3	15.3	1.33
Alloy K	20.3	14.6	1.39

FIG. 3B

Alloy	As Cast Microstructure			New PHACOMP Analysis (Annealing Temp = 1050°C)				
	% δ (DeLong)	Mode	M _d Temp (°C)	Cr ₂ N Phase	σ Phase	Md ^{ave} (eV)	Md ^{crit} (eV)	Max N Sol. (%)
Alloy E	2	AF	-147.1	No	No	0.921	0.925 (2)	0.42
Alloy F	3	AF	-147.1	No	No	0.923	0.926 (2)	0.45
Alloy G	4	AF	-2.6	No	No	0.910	0.917 (1)	0.30
Alloy H	5	AF	-2.6	No	No	0.912	0.917 (1)	0.33
Alloy I	3	AF	-67.6	No	Borderline*	0.916	0.917 (1)	0.37
Alloy J	2	AF	-168.2	No	No	0.922	0.925 (2)	0.43
Alloy K	4	AF/FA	-168.2	No	Borderline*	0.928	0.927 (2)	0.51

FIG. 3C

*: $\Delta < 0.002$

Alloy	Mechanical (Annealed – 1050°C)		Corrosion PRE	Radiopacity Change from 316LS (Thickness = 0.005")			
	Yield Strength (MPa)	UTS (MPa)		40 keV	60 keV	80 keV	100 keV
				(%)	(%)	(%)	(%)
Alloy E	406	744	-	+4.6	+1.6	+5.0	+2.8
Alloy F	406	732	29.1	+4.3	+1.6	+4.9	+2.7
Alloy G	307	651	29.1	+7.0	+2.4	+5.5	+3.1
Alloy H	307	639	28.2	+6.8	+2.3	+5.4	+3.0
Alloy I	307	710	28.2	+15.5	+5.2	+12.2	+6.8
Alloy J	378	767	28.1	+13.5	+4.6	+11.7	+6.5
Alloy K	378	742	28.1	+12.9	+4.4	+11.5	+6.3

FIG 3D

FIG. 3D

Alloy	Elemental Composition (wt %)															
	Ni	Cr	Mn	C	Mo	Si	N	Co	Pt	Ru	Pd	Ir	Rh	Au	Cu	Fe
Alloy L	0	18	1.5	0.03	2.8	0.2	0.06	10	25	0	0	0	0	0	0.09	Balance
Alloy M	0	18	1.5	0.03	2.8	0.2	0.06	12.5	22.5	0	0	0	0	0	0.09	Balance
Alloy N	0	18	1.5	0.03	2.8	0.2	0.06	15	20	0	0	0	0	0	0.09	Balance
Alloy O	0	18	1.5	0.03	2.8	0.2	0.06	17.5	17.5	0	0	0	0	0	0.09	Balance
Alloy P	0	18	1.5	0.03	2.8	0.2	0.06	20	15	0	0	0	0	0	0.09	Balance
Alloy Q	0	18	1.5	0.03	2.8	0.2	0.06	22.5	12.5	0	0	0	0	0	0.09	Balance

FIG. 4A

Alloy	Cr Equivalent	Ni Equivalent	Cr _{eq} /Ni _{eq}
Alloy L	21.5	18.7	1.15
Alloy M	21.5	18.6	1.16
Alloy N	21.5	18.4	1.16
Alloy O	21.5	18.3	1.17
Alloy P	21.5	18.3	1.18
Alloy Q	21.5	18.1	1.19

FIG. 4B

Alloy	As Cast Microstructure			New PHACOMP Analysis (Annealing Temp = 1050°C)				
	% δ (DeLong)	Mode	M _d Temp (°C)	Cr ₂ N Phase	σ Phase	Md ^{ave} (eV)	Md ^{crit} (eV)	Max N Sol. (%)
Alloy L	0	A	-192.6	No	Yes	0.925	0.917 (1)	0.47
Alloy M	0	A	-167.6	No	Yes	0.922	0.917 (1)	0.43
Alloy N	0	A	-142.6	No	Borderline	0.919	0.917 (1)	0.40
Alloy O	0	A	-117.6	No	Borderline	0.917	0.917 (1)	0.37
Alloy P	0	A	-92.6	No	No	0.914	0.917 (1)	0.34
Alloy Q	0	A	-67.6	No	No	0.912	0.917 (1)	0.32

FIG. 4C

Alloy	Mechanical (Annealed-1050 °C)		Corrosion	Radiopacity Change from 316LS (Thickness = 0.005")							
	Yield Strength (MPa)	UTS (MPa)		40 keV		60 keV		80 keV		100 keV	
						%	%	%	%	%	%
Alloy L	307	822	28.2			37.2	11.8	28.3			15.3
Alloy M	307	800	28.2			32.4	10.4	24.7			13.4
Alloy N	307	777	28.2			28.0	9.1	21.4			11.7
Alloy O	307	755	28.2			23.8	7.8	18.2			10.0
Alloy P	307	732	28.2			19.9	6.6	15.2			8.4
Alloy Q	307	710	28.2			16.2	5.4	12.3			6.9

FIG. 4D

INTERNATIONAL SEARCH REPORT

ational Application No

PC/US 03/41462

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 A61L31/02 A61L31/18

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61L

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, WPI Data, PAJ, INSPEC, MEDLINE, BIOSIS, COMPENDEX

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 02/078764 A (SCIMED LIFE SYSTEMS INC) 10 October 2002 (2002-10-10) page 3, line 9 - line 30 page 4, line 16 - line 20 claim 1	1-51
X	US 6 267 921 B1 (MONTAGNON JACQUES ET AL) 31 July 2001 (2001-07-31) column 1, line 6 - line 13 column 1, line 65 - column 2, line 8 claims ----- -/-	1-10, 15-23, 26, 31-37, 46-49,51

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents:

A document defining the general state of the art which is not considered to be of particular relevance

E earlier document but published on or after the international filing date

L document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

O document referring to an oral disclosure, use, exhibition or other means

P document published prior to the international filing date but later than the priority date claimed

T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

X document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

Y document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

G document member of the same patent family

Date of the actual completion of the international search

8 June 2004

Date of mailing of the international search report

17/06/2004

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax (+31-70) 340-3016

Authorized officer

Muñoz, M

INTERNATIONAL SEARCH REPORT

International Application No
PCT/US 03/41462

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	<p>GEBEAU R C ET AL: "Biomedical implant alloy"</p> <p>ADV MATER PROCESSES; ADVANCED MATERIALS AND PROCESSES SEPTEMBER 2001, vol. 159, no. 9, September 2001 (2001-09), pages 46-48, XP008031325</p> <p>the whole document</p>	46-49
X	<p>WO 01/41829 A (ADVANCED CARDIOVASCULAR SYSTEM) 14 June 2001 (2001-06-14)</p> <p>page 8, line 8 - page 9</p>	46-49

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 03/41462

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 02078764	A	10-10-2002	US 2002193865 A1	19-12-2002
			US 2003018380 A1	23-01-2003
			CA 2442200 A1	10-10-2002
			CA 2442205 A1	10-10-2002
			EP 1372754 A1	02-01-2004
			EP 1404391 A1	07-04-2004
			WO 02078763 A1	10-10-2002
			WO 02078764 A1	10-10-2002
			US 2003077200 A1	24-04-2003
US 6267921	B1	31-07-2001	FR 2764307 A1	11-12-1998
			AT 210202 T	15-12-2001
			DE 69802837 D1	17-01-2002
			DE 69802837 T2	27-06-2002
			EP 1025273 A1	09-08-2000
			WO 9855662 A1	10-12-1998
			JP 2002502464 T	22-01-2002
WO 0141829	A	14-06-2001	US 6508832 B1	21-01-2003
			AU 1941301 A	18-06-2001
			WO 0141829 A1	14-06-2001
			US 2003106218 A1	12-06-2003

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ **BLACK BORDERS**
- ☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- ☐ **FADED TEXT OR DRAWING**
- ☐ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- ☐ **SKEWED/SLANTED IMAGES**
- ☐ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- ☐ **GRAY SCALE DOCUMENTS**
- ☐ **LINES OR MARKS ON ORIGINAL DOCUMENT**
- ☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**
- ☐ **OTHER:** _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.

This Page Blank (uspto)